

Hello Bio, Inc.
304 Wall St., Princeton, NJ 08540 USA

T. 609-683-7500
F. 609-228-4994

customercare-usa@m2stage.hellobio.com



DATASHEET

MightyMount™ Antifade Fluorescence Mounting Medium (hardset)

Product overview

Name	MightyMount™ Antifade Fluorescence Mounting Medium (hardset)
Cat No	HB6966
Biological description	Overview

MightyMount™ Antifade Fluorescence Mounting Medium (hardset) is an ideal formulation for prevention of photobleaching of fluorescent proteins and dyes during fluorescent imaging. It is easy to use with an ideal refractive index and provides effective prevention of photobleaching.

Applications: IHC(IF), ICC, Cellular imaging, Super-resolution microscopy

Mounting: Aqueous (hardset) - cures in approximately 1 hour at room temperature

Antifade: Yes

Counterstain: None

Refractive index: ≈1.45 (initial) which then increases to ≈1.518 once cured

Other Mounting Media Products

We supply a full range of mounting media for a range of experimental needs:

Hardset:

- HB8459 - MightyMount™ Antifade Fluorescence Mounting Medium with DAPI (hardset)
- HB7033 - MightyMount™ Antifade Fluorescence Mounting Medium with Propidium Iodide (hardset)
- HB7508 - MightyMount™ Antifade Fluorescence Mounting Medium with Phalloidin-TRITC (hardset)


Aqueous:

- HB9854 - MightyMount™ Antifade Fluorescence Mounting Medium (aqueous)
- HB7618 - MightyMount™ Antifade Fluorescence Mounting Medium with DAPI (aqueous)
- HB8761 - MightyMount™ Antifade Fluorescence Mounting Medium with Propidium Iodide (aqueous)
- HB9417 - MightyMount™ Antifade Fluorescence Mounting Medium with Phalloidin-TRITC (aqueous)

Applications
Description

ICC, IF, IHC(IF)
Antifade fluorescence hard-set mounting medium for use in IHC(IF) and ICC.

Images

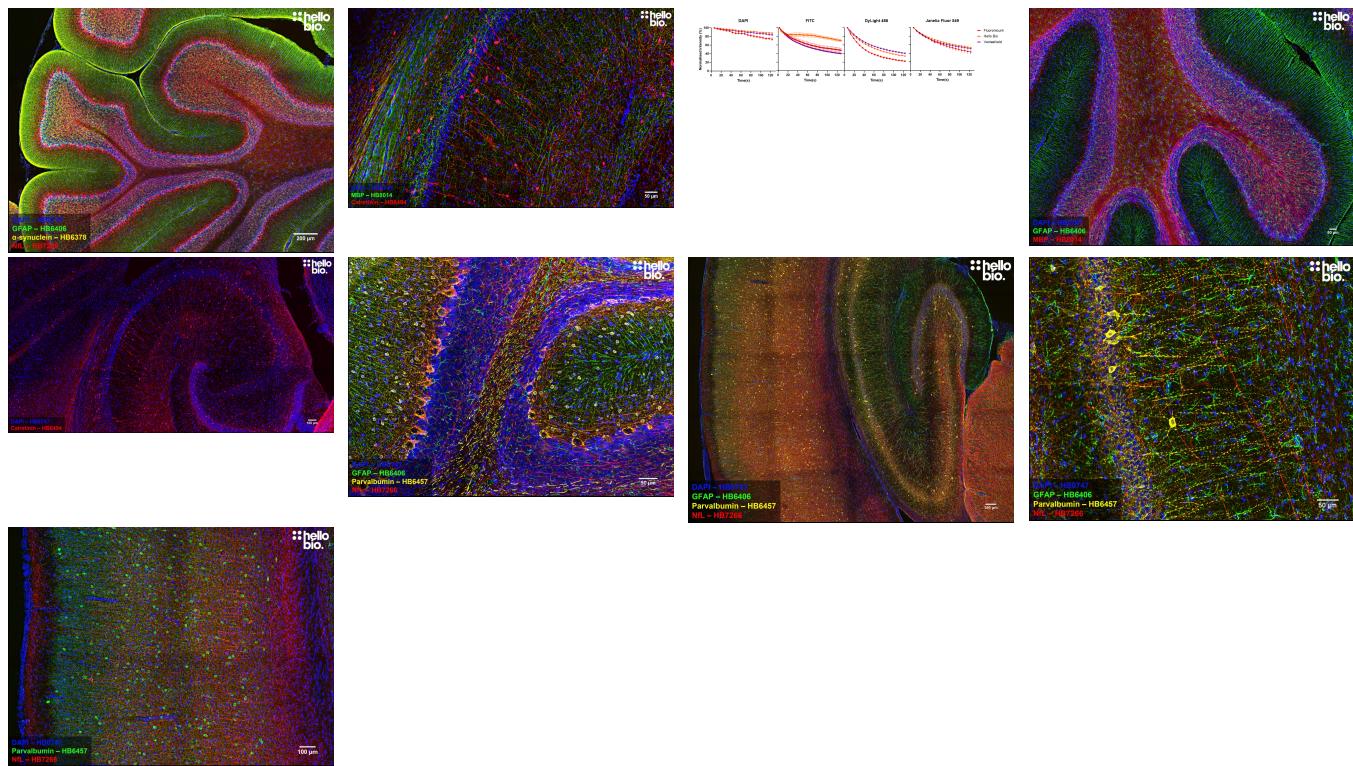

Biological Data

Application notes

Protocol for use of mounting media Once mounted, store slides at 4°C in the dark for optimal preservation of fluorescence.

IHC(IF)

1. Mount sections onto subbed or charged microscope slides and air dry (in the dark) until sections are moist but all excess liquid has evaporated
2. Add a few drops of mounting media around the sections (around 50µl but this will depend on the number and thickness of sections) and slowly lower the coverslip from one end of the slide to the other being careful to avoid creating any bubbles.
3. Wrap slides in foil to prevent light exposure then allow the media to cure at 4°C overnight before imaging. If more rapid imaging is needed it is possible to accelerate the curing process by incubating slides at either room temperature or 37°C for ≈1 hour.

For more information on IHC(IF) including tips on how to mount sections, please see our [IHC\(IF\) protocol](#)

ICC

1. Add a drop of mounting medium (Around 5µl for a 10mm and 15µl for a 22mm coverslip) to a standard microscope slide.
2. Briefly rinse the coverslip in dH₂O before placing face down into the drop of mounting medium being careful not to introduce bubbles.
3. Wrap slides in foil to prevent light exposure then allow the media to cure at 4°C overnight before imaging. If more rapid imaging is needed it is possible to accelerate the curing process by incubating slides at either room temperature or 37°C for ≈1 hour.

For more information on ICC please see our [ICC protocol](#)

Solubility & Handling

Storage instructions

+4°C. Protect from light.

Storage buffer

Contains 0.05% sodium azide

Storage instructions

+4°C. Protect from light.

Important

This product is for RESEARCH USE ONLY and is not intended for therapeutic or diagnostic use. Not for human or veterinary use.
